

GUIDELINES FOR AUTOSAMPLER VIAL SELECTION

We have updated this section to make it easier to select the appropriate vials and/or accessories quickly and accurately.
All the seals, caps, septa and inserts will be located on the corresponding vial pages.



Vial Description

Vial Dimensions Neck Finish Closure size	12x32 Crimp 11mm	12x32 Screw 8-425	12x32 Screw 9-425	12x32 Screw 10-425	12x32 Snap Snap	15x45 Screw 13-425	15x45 Shell	8x40 Shell	8x40 Crimp 9mm	Headspace Crimp 20mm	Headspace Screw
Autosampler	See Page										
Agilent 1050, 1090, 1100 5890, 6890, 7890 7673 A/B, 7683 B Headspace	305-310	316-317	305, 314-315	318	305, 311-313					322	322
Beckman 501, 502, 507		316-317	305, 314-315	318					321		
Hitachi AS-2000, AS-6000 S6551, L-7200 L-7250	305-310	316-317 316-317 316-317	305, 314-315 305, 314-315 305, 314-315		305, 311-313						
Konik HRGC4000 B	305-310	316-317									
Leap CTC A200S Headspace	305-310	316-317	305, 314-315	318	305, 311-313					322	
Perkin Elmer Autosystem LC600 42 vial tray 420/B, 4900 Headspace	305-310 305-310 305-310	316-317	305, 314-315		305, 311-313					322	
Shimadzu SIL-6B, -7A, -8A SIL10A, 10Ai, 10AxL SIL-2AS	305-311	316-317	318								
Spark Holland Marathon Promis Triathlon Midas	305-310 305-310 305-310 305-310	316-317 316-317 316-317 316-317	305, 314-315 305, 314-315	318	305, 311-313 305, 311-313						
Spectra Physics/Thermo 8875, 8880	305-310	316-317	305, 314-315		305, 311-313						
Varian 8000 series 8100/8200 Marathon 9100/9090/9095 Headspace	305-310 305-310 305-310	316-317 316-317 316-317 316-317	305-314-315 305-314-315	318	305, 311-313				321		
Waters Alliance 2690 Wisp 717 48 position Wisp 717 96 position			305, 314-315	318		319	320	320			

If you don't see your instrument listed in the table above, contact our Technical Support Team at 1-800-267-8103 for assistance or to try a sample.

1-800-267-8103

Chromatographic Specialties Inc.

GUIDELINES FOR AUTOSAMPLER VIAL SELECTION

A VIAL IS A VIAL, OR IS IT?

Autosampler vials may seem insignificant when compared to the sophisticated analytical instrumentation most laboratories use, but the incorrect vial, cap or septa can contribute to problems that can decrease productivity and reproducibility.

Potential Problems Caused by Using Incorrect Vial/Cap/Septum:

- Loss of analyte due to evaporation
- Presence of extra peaks in the chromatogram due to solvent/septum interaction
- Mechanical damage to autosampler
- Sample degradation
- Irreproducible injection volumes



WHAT TO CONSIDER WHEN SELECTING AN AUTOSAMPLER VIAL

Autosampler Compatibility

Not all autosamplers are alike. Some utilize robotic arms to pick up a sample vial; some use tray rotation while others move the sampling needle to the respective vial coordinates. The dimensions of autosampler vials vary. Most autosamplers are equipped with trays that use 12x32mm vial configurations but some like the Waters Wisp require a 15x45mm configuration. Consult your autosampler's operating manual or manufacturer to determine the vial dimensions required.

Sample Volume

The amount of sample available for analysis is important in choosing the appropriate vial. If only a limited volume of sample is available, you will have to choose between using an insert for your regular autosampler vial, a microvial or a high recovery vial.

Note: Most 12x32 mm autosampler vials hold between 1.5mL to 2.0mL of liquid, depending on where the manufacture measures the vial full. The dimensions for 12x32mm vials are standard between manufacturers but the length of the neck and width/shape of the vial shoulder may vary. 12x32mm microvials have the same outer dimensions but the inside of the vial may be tapered to reduce volume or contain a fused insert. 12x32mm high recovery vials will have an internal conical bottom that allows for maximum sample recovery.

Sample Compatibility

The analyte and solvent compatibility should be considered in choosing vials and accessories. For example, amber glass is most often used for light sensitive samples while deactivated glass or plastic vials are used for compounds that are sensitive to glass or stick to the glass itself. Volatile samples require closures that reduce the risk of analyte loss due to evaporation.

Vial Composition

Several factors need to be considered when choosing laboratory glass - chemical inertness, durability, light sensitivity, storage conditions, analyte composition and especially exposure to heat/freezing temperatures.

Linear Coefficient of Expansion refers to the fractional change in the length of glass per degree of change in temperature, in short, the ability of the glass to tolerate rapid thermal changes. The lower the coefficient of expansion the better the glass can handle temperature change without fracturing.

Classifications for laboratory glass based on its resistance to attack from water were established by the United States Pharmacopoeia, USP.

USP Type 1, Class A, 33 Borosilicate Glass is the most inert and chemically resistant glass widely used in laboratories especially for chromatography applications. Type I glass is composed primarily of silicone and oxygen, with trace amounts of boron and sodium. It has the lowest leaching characteristics and a linear coefficient of expansion of 33.

USP Type 1, Class B, 51 Borosilicate Glass which is composed of silicone and oxygen, trace amounts of boron, sodium and other element is more alkaline than Class A glass but still adequate for laboratory use. All amber borosilicate glass is made of Class B unless otherwise specified and has an expansion coefficient of 51.

Silanized or deactivated glass is borosilicate glass that has undergone further deactivation by treating the surface of the glass with an organosilane. The surface becomes more hydrophobic and inert making the vial suitable for use with pH sensitive compounds, trace analyses and applications requiring long term sample storage.

GUIDELINES FOR AUTOSAMPLER VIAL SELECTION



USP Types II, III and NP glass are manufactured from soda lime which has less chemical resistance than borosilicate.

Polypropylene is a rigid and translucent material, which also comes in a variety of colours and has good chemical resistance for short term storage of most common laboratory chemicals. Resistance decreases over time when using aromatic and halogenated hydrocarbons. Polypropylene vials are often used for ion chromatography because of the extremely low metal content and excellent cleanability with dilute acid followed by deionized water rinse. Polypropylene vials limit the exposure to hazardous materials since they can be incinerated while sealed.



Polymethylpentene (TPX) is a rigid transparent material, which has a relatively high melting point with a temperature range of 0°-170°C. TPX vials can be used as alternative to opaque polypropylene vials because they provide maximum clarity. Their chemical resistance is similar to that of polypropylene vials. TPX vials should be used for applications where visual clarity is required or repetitive exposure to higher temperatures such as autoclaving. TPX vials tend to be more brittle at room temperature.



Type of Vial Finish and Closures

Autosampler vials are available in a variety of neck finishes and opening diameters. Large mouth or wide ID vials have approximately a 40% wider mouth opening than standard opening vials. The large opening reduces the risk of bent autosampler needles during sampling.



Screw thread vials and caps provide low evaporation, reusability, less hand injury during manipulation than crimp seals and require no special tools. All screw threads vials and caps are differentiated by their thread finish as defined by the Glass Packaging Institute, GPI. For screw thread vials, a two part number is assigned. For example, 8-425 neck finish represents a vial with a diameter of 8 mm across the outside of the threads and a thread style of 425. Screw thread vials and caps are more expensive than crimp seals.



Caps for screw thread vials are available with either an open hole for autosampler use and standard addition or with a solid top for sample storage. One piece polypropylene cap and membrane are also available. These pierceable screw thread caps are designed for one time use and reduce sample preparation time as there is no cap and seal to assemble.

Crimp top vials require lacquered aluminum crimp seals which are relatively inexpensive and, when properly assembled, provide the best seal for long term storage. Crimp seals are not reusable.



A **crimping tool** is required to seal caps and a decrimper or decapper is required to remove the seals. Several types of hand crimpers are available including the adjustable precision crimpers that Chromatographic Specialties offers. Adjustable hand crimpers feature an adjustable stop on the handle to provide consistent seal tightness every time. Adjusting the hex screw inside the steel crimper jaws will also alter the amount of crimp. Achieving a good crimp is crucial because overcrimping can cause septum coring, bent needles and create a larger hole in the PTFE septum layer than a properly crimped seal. Undercrimping can result in loose seals and sample evaporation.

Hand decrimpers quickly and safely remove seals with just a single squeeze of the handle. Decappers are similar in design to pliers and provide an inexpensive alternative to decrimpers. Decrimpers should be used for applications involving hazardous samples because there is less chance of spillage.

Electronic crimpers and decappers are also available. Electronic units reduce hand fatigue, provide consistent crimps and are ideal for laboratories analyzing a lot of samples.


Snap seal vials are less prone to breakage during decapping because more glass is used in the neck of the vial. The snap seal neck finish is compatible with either crimp and/or snap seals and no special tools are required to remove the cap. These vials are recommended for short term sample storage and non-volatile samples because the seal is not as secure as a crimp or screw thread seal.



Shell Vials are an economical alternative to screw thread vials for Waters' HPLC autosamplers or any other autosampler that doesn't use a robotic arm to move the vials. Most shell vials are sold with a polyethylene cap that has a starburst design for easy needle penetration.

GUIDELINES FOR AUTOSAMPLER VIAL SELECTION

WHAT TO CONSIDER WHEN SELECTING THE PROPER INSERT...

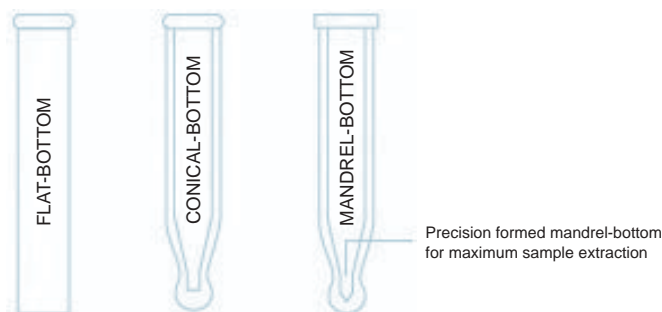

Limited volume inserts are an economical solution when there is a limited amount of sample and injection is done using an autosampler. Most autosamplers have a set depth that the injection needle can go into the vial without bottoming out. Inserts increase the sample depth within the vial even if there is a very minute volume of sample available.

Solvent Compatibility

Type I borosilicate glass inserts are most commonly used for trace analysis in chromatography.

Polypropylene inserts are less expensive than glass and are suitable for applications involving pH sensitive samples.

Insert Shape and Point Style

The style of insert chosen is dependent on the amount of sample available and the residual volume after sampling.

- **Conical** inserts have a tapered bottom with pulled tips and are available with or without plastics springs. The spring acts as a shock absorber during needle penetration and raises the insert above the bottom of the vial, allowing greater sample recovery.
- **Mandrel** inserts also have a tapered bottom but the tips have been precision formed over a mandrel to give the internal tip a "V" shape that reduces the residual volume of the insert. Mandrel precision formed inserts are recommended when maximum recovery of the sample is required.
- **Flat bottom** inserts have the largest capacity and are the most economical inserts. These inserts are cylindrical in shape with a flat bottom
- **Hanging** inserts have either a flange top or top spring that suspends the insert correctly centered in the vial.
- **Step** inserts with a built-in glass flange are designed specifically for step vials with a special tapered neck. The flange suspends the insert correctly centered in the vial without causing a bulge in the septum when the cap is screwed on.

Dimensions of the Autosampler Vial

Choosing the incorrect size of insert for an autosampler vial can result in poor reproducibility between sample injections, damage to the autosampler needle and an inadequate seal between the septum and the vial. The dimensions listed for insert size in the catalogue refer to the outside diameter and length. Inserts with an outside diameter of 5mm are used with vials with standard mouth openings and the 6mm are used with wide mouth vials. The length of the insert should be flush with the neck of the vial to prevent the insert from causing the septum to bulge.

DIRECT
613-342-4678

TOLL FREE
800-267-8103

FAX
613-342-1144

TECHNICAL SUPPORT
tech@chromspec.com

www.chromspec.com
GENERAL INQUIRIES
sales@chromspec.com

INSTRUMENTATION
instrum@chromspec.com

GUIDELINES FOR AUTOSAMPLER VIAL SELECTION

WHAT TO CONSIDER WHEN SELECTING SEPTA



Septum compatibility or chemical resistance with the sample and solvent is the main consideration when choosing vial septa. Any interaction can lead to sample degradation or the appearance of ghost peaks in the chromatogram. PTFE is the most inert but has poor resealability making it unsuitable for multiple injections or storage. For layered septa such as PTFE/silicone the chemical resistance of the septa is that of PTFE until the septum is punctured. Once punctured, the silicone layer is exposed and able to react with sample/solvent so the chemical resistance of silicone should be considered when using these septa.

Note: The thicker the facings on the seal the better the resealability but it compromises the ability of the autosampler needle to pierce the septum.

Septa Material	Advantages	Chemical Resistance	Applications	Max Temp
PTFE	Economical	Excellent	For single injection only	550°C
PTFE/silicone	Excellent resealing capabilities	Excellent until punctured Not suitable for chlorosilanes	Multiple injections than moderate resistance	200°C
Pre-slit PTFE/silicone	Reduces coring Prevents vacuum from inside the vial	Excellent until punctured than moderate resistance	Multiple injections	200°C
PTFE/silicone/PTFE	Resistant to coring Autoclavable	Excellent	Above average resealing Multiple injections or applications with long periods between injections	200°C
PTFE/red rubber	Economical	Excellent until punctured	Moderate resealability not recommended for holding samples for further analysis	110°C
Molded polypropylene	Economical	Good Not resealable	For single injection use only	130°C
Gray butyl	Very economical	Not suitable for chlorinated solvents, alkanes, benzenes or cyclohexanes	Suitable for low pressure applications	125°C
Viton		Excellent chemical resistance Good for chlorinated solvents Not recommended for use with amines, pyridine, acetonitrile, DMF, DMSO, THF, dioxane, methanol, Freon 22, ethylacetate, acetone or acid anhydrides.	Average resealability	160°C